RETURN TO PRODUCT BULLETIN TABLE OF CONTENTS
RETURN TO CD-ROM TABLE OF CONTENTS

North American Dräger

PRODUCT BULLETIN

Product(s):	Narkomed 6000
Bulletin Number:	080
Release Date:	May 24, 1999
Pages:	1

Subject: AUDIP Indicator Software Option

In addition to the standard pressure monitoring capabilities, an Audible Pressure Gauge (AUDIP) Indicator is being offered as a software option designed for the Narkomed 6000 to provide graphic, numeric, and audio signaling. Activation of this feature will be through the Utilities Notebook or through a shortcut key in the control bar at the bottom of the main display.

The indicator incorporates a circular analog gauge and large numeric values for instantaneous pressure, peak pressure, and PEEP.

The indicator can also be configured to provide an audio tone when a pressure threshold is reached (e.g. to maintain pressure below 20 cmH_2O for LMA cases). This audio capability is activated through the audio speaker icon on the face of the gauge. The audio pressure threshold is adjusted by using the up and down arrows; the default threshold is 20 cmH_2O. When the audio tone is enable, a gray line appears extending from the center of the gauge to indicate the audio tone's set threshold value. This threshold value is also displayed in numerics in the center of the gauge. The volume of the audio tone may be adjusted through the Volume tab on the System Setup Notebook.

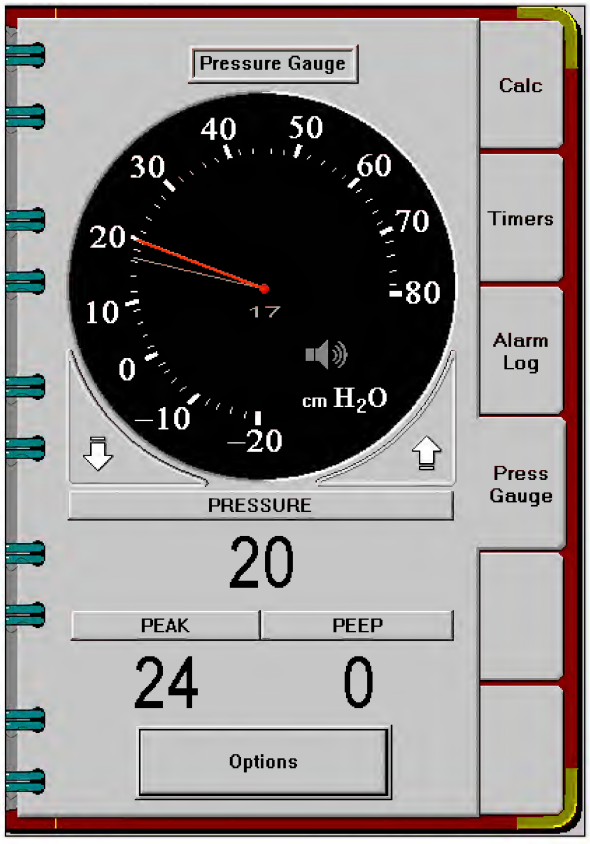

The list price for this feature is $195.

NAD is offering this feature as a free upgrade to all installed base Narkomed 6000 customers in appreciation for their valuable feedback. This offer will be extended to all Narkomed 6000 customers who purchase prior to September 30, 1999.

Additional details are provided in the Narkomed 6000 Operator's Manual. If you have any questions or require further information, please contact Debbie DeColli at x2510.